

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02274 Calib. Date: 12/08/2014 Calib. No.: 00025
Certification File No.: 02275 Cert. Date: 12/08/2014 Cert. No.: 00022
Linearity File No.: 02276 Lin. Date: 12/08/2014 Lin. No.: 00021
Solution File No.: 02289 Soln. Date: 01/05/2015 Soln. No.: 00220
Sequential File No.: 02289 File Date: 01/05/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1318

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:36S		
Control 1 EC	0.101%	20:37S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:37S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38S		
Control 2 EC	0.098%	20:38S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:39S		
Control 3 EC	0.099%	20:40S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:41S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Sgt. M Henkel 149

Badge No.: 149

Date: 01/05/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02274 Calib. Date: 12/08/2014 Calib. No.: 00025
Certification File No.: 02275 Cert. Date: 12/08/2014 Cert. No.: 00022
Linearity File No.: 02276 Lin. Date: 12/08/2014 Lin. No.: 00021
Solution File No.: 02294 Soln. Date: 02/01/2015 Soln. No.: 00221
Sequential File No.: 02294 File Date: 02/01/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1314

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:20S		
Control 1 EC	0.101%	17:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	17:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:21S		
Control 2 EC	0.097%	17:22S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:23S		
Control 3 EC	0.098%	17:24S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:25S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: REESE

First Name: STEVEN

MI: R

Signature: Prz S Reese

Badge No.: 137

Date: 02/01/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02274	Calib. Date: 12/08/2014
Certification File No.:	02275	Calib. No.: 00025
Linearity File No.:	02276	Cert. Date: 12/08/2014
Solution File No.:	02299	Cert. No.: 00022
Sequential File No.:	02299	Lin. Date: 12/08/2014
		Lin. No.: 00021
		Soln. Date: 02/14/2015
		Soln. No.: 00222
		File Date: 02/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 1308

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:04S		
Control 1 EC	0.099%	20:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06S		
Control 2 EC	0.096%	20:06S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:07S		
Control 3 EC	0.097%	20:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

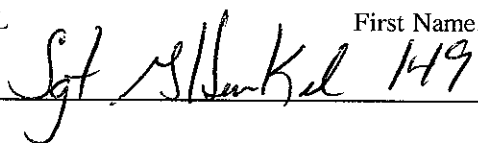

Badge No.: 149

Date: 02/14/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02274 Calib. Date: 12/08/2014 Calib. No.: 00025
Certification File No.: 02275 Cert. Date: 12/08/2014 Cert. No.: 00022
Linearity File No.: 02276 Lin. Date: 12/08/2014 Lin. No.: 00021
Solution File No.: 02302 Soln. Date: 02/22/2015 Soln. No.: 00223
Sequential File No.: 02302 File Date: 02/22/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1310

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:11S		
Control 1 EC	0.100%	06:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13S		
Control 2 EC	0.098%	06:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:14S		
Control 3 EC	0.098%	06:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

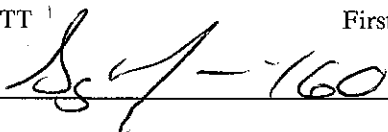

Badge No.: 160

Date: 02/22/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02306 Calib. Date: 03/31/2015 Calib. No.: 00027
Certification File No.: 02307 Cert. Date: 03/31/2015 Cert. No.: 00023
Linearity File No.: 02308 Lin. Date: 03/31/2015 Lin. No.: 00022
Solution File No.: 02312 Soln. Date: 05/02/2015 Soln. No.: 00226
Sequential File No.: 02312 File Date: 05/02/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1319

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:19D		
Control 1 EC	0.101%	13:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		
Control 2 EC	0.100%	13:21D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21D		
Control 3 EC	0.099%	13:22D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 05/02/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02321	Calib. Date: 06/09/2015
Certification File No.:	02322	Calib. No.: 00028
Linearity File No.:	02323	Cert. Date: 06/09/2015
Solution File No.:	02336	Cert. No.: 00024
Sequential File No.:	02336	Lin. Date: 06/09/2015
		Lin. No.: 00023
		Soln. Date: 07/10/2015
		Soln. No.: 00228
		File Date: 07/10/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 1325

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:48D		
Control 1 EC	0.099%	00:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	00:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:49D		
Control 2 EC	0.099%	00:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:51D		
Control 3 EC	0.099%	00:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SEXTON

First Name: RYAN

MI: G

Signature: _____

Handwritten signature #206

Badge No.: 206

Date: 07/10/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02321	Calib. Date:	06/09/2015
Certification File No.:	02322	Cert. Date:	06/09/2015
Linearity File No.:	02323	Lin. Date:	06/09/2015
Solution File No.:	02348	Soln. Date:	08/07/2015
Sequential File No.:	02348	File Date:	08/07/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	1304

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:58D		
Control 1 EC	----%	17:58D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	----%	17:58D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	----%	--:--		
Control 2 EC	----%	--:--	N/A	
Control 2 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		
Control 3 EC	----%	--:--	N/A	
Control 3 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: Sgt M Henkel 149

Badge No.: 149

Date: 08/07/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02321	Calib. Date:	06/09/2015
Certification File No.:	02322	Cert. No.:	00028
Linearity File No.:	02323	Cert. Date:	06/09/2015
Solution File No.:	02349	Lin. No.:	00023
Sequential File No.:	02349	Soln. Date:	08/08/2015
		Soln. No.:	00230
		File Date:	08/08/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	14L135	Expires:	12/21/2016
		Bottle No.:	0059

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:25D		
Control 1 EC	0.100%	20:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:26D		
Control 2 EC	0.099%	20:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:27D		
Control 3 EC	0.099%	20:28D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Sgt M Henkel 149

Badge No.: 149

Date: 08/08/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02321	Calib. Date: 06/09/2015
Certification File No.:	02322	Calib. No.: 00028
Linearity File No.:	02323	Cert. Date: 06/09/2015
Solution File No.:	02361	Cert. No.: 00024
Sequential File No.:	02361	Lin. Date: 06/09/2015
		Lin. No.: 00023
		Soln. Date: 09/09/2015
		Soln. No.: 00231
		File Date: 09/09/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0062

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:07D		
Control 1 EC	0.101%	10:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08D		
Control 2 EC	0.100%	10:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:10D		
Control 3 EC	0.101%	10:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	10:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P

Signature: *Tr. I. Michael P. Gibson #6353*

Badge No.: 6353

Date: 09/09/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02321 Calib. Date: 06/09/2015 Calib. No.: 00028
Certification File No.: 02322 Cert. Date: 06/09/2015 Cert. No.: 00024
Linearity File No.: 02323 Lin. Date: 06/09/2015 Lin. No.: 00023
Solution File No.: 02371 Soln. Date: 10/16/2015 Soln. No.: 00233
Sequential File No.: 02371 File Date: 10/16/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 12/31/2016
Solution Control Lot: 14L135 Bottle No.: 0057

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:16D		
Control 1 EC	0.101%	12:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:17D		
Control 2 EC	0.100%	12:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		
Control 3 EC	0.101%	12:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:20D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

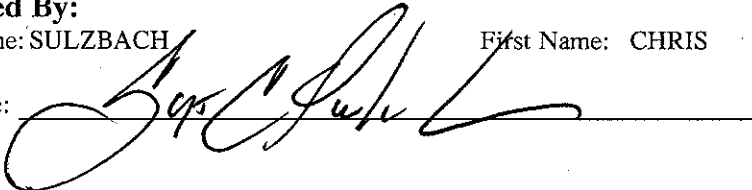Signature: 

Badge No.: 127

Date: 10/16/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02321	Calib. Date: 06/09/2015
Certification File No.:	02322	Calib. No.: 00028
Linearity File No.:	02323	Cert. Date: 06/09/2015
Solution File No.:	02376	Cert. No.: 00024
Sequential File No.:	02376	Lin. Date: 06/09/2015
		Lin. No.: 00023
		Soln. Date: 11/14/2015
		Soln. No.: 00234
		File Date: 11/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0053

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:29S		
Control 1 EC	0.103%	08:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	08:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:31S		
Control 2 EC	0.102%	08:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	08:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:32S		
Control 3 EC	0.103%	08:32S	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.105%	08:32S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:33S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] #187

Badge No.: 187

Date: 11/14/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02321	Calib. Date: 06/09/2015
Certification File No.:	02322	Calib. No.: 00028
Linearity File No.:	02323	Cert. Date: 06/09/2015
Solution File No.:	02378	Cert. No.: 00024
Sequential File No.:	02378	Lin. Date: 06/09/2015
		Lin. No.: 00023
		Soln. Date: 11/14/2015
		Soln. No.: 00236
		File Date: 11/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0054

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:32S		
Control 1 EC	0.104%	14:32S	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.106%	14:32S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	14:33S		
Control 2 EC	0.103%	14:34S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	14:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:35S		
Control 3 EC	0.103%	14:35S	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.105%	14:35S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	14:36S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] #187

Badge No.: 187

Date: 11/14/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02321	Calib. Date: 06/09/2015
Certification File No.:	02322	Calib. No.: 00028
Linearity File No.:	02323	Cert. Date: 06/09/2015
Solution File No.:	02377	Cert. No.: 00024
Sequential File No.:	02377	Lin. Date: 06/09/2015
		Lin. No.: 00023
		Soln. Date: 11/14/2015
		Soln. No.: 00235
		File Date: 11/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0058

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:53S		
Control 1 EC	0.104%	11:54S	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.105%	11:54S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:55S		
Control 2 EC	0.102%	11:55S	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.105%	11:55S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:56S		
Control 3 EC	0.103%	11:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 11/14/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02321	Calib. Date:	06/09/2015
Certification File No.:	02322	Cert. No.:	00028
Linearity File No.:	02323	Cert. Date:	06/09/2015
Solution File No.:	02379	Lin. No.:	00023
Sequential File No.:	02379	Soln. Date:	11/15/2015
		Soln. No.:	00237
		File Date:	11/15/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	14L135	Expires:	12/31/2016
		Bottle No.:	0055

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:05S		
Control 1 EC	0.104%	08:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	08:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07S		
Control 2 EC	0.103%	08:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	08:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08S		
Control 3 EC	0.103%	08:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.105%	08:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

 *157

Badge No.: 187

Date: 11/15/2015

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02382	Calib. Date: 11/25/2015
Certification File No.:	02383	Calib. No.: 00029
Linearity File No.:	02384	Cert. Date: 11/25/2015
Solution File No.:	02389	Cert. No.: 00025
Sequential File No.:	02389	Lin. Date: 11/25/2015
		Lin. No.: 00024
		Soln. Date: 12/26/2015
		Soln. No.: 00239
		File Date: 12/26/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0060

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:00S		
Control 1 EC	0.100%	13:01S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:02S		
Control 2 EC	0.098%	13:02S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:03S		
Control 3 EC	0.099%	13:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 12/26/2015