

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Location: PENNSAUKEN TWSP. P.D. Serial No.: ARUM-0051
Calibration File No.: 02684 Calib. Date: 11/27/2017 Calib. No.: 00034
Certification File No.: 02637 Cert. Date: 07/11/2017 Cert. No.: 00029
Linearity File No.: 02638 Lin. Date: 07/11/2017 Lin. No.: 00028
Solution File No.: 02683 Soln. Date: 11/17/2017 Soln. No.: 00281
Sequential File No.: 02684 File Date: 11/27/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 10/10/2018
Solution Control Lot: 16270 Bottle No.: 1055

Coordinator

Last Name: WATSON First Name: MATTHEW MI: R
Signature: Tpr. II *Matthew J. Walsh* #7078 Badge No.: 7078
Date: 11/27/2017

*Black Key Temperature Probe Serial.....# DDXKP2-398 (MRW)
*Digital NIST Temperature Measuring System Serial.....# 170428362 (MRW)

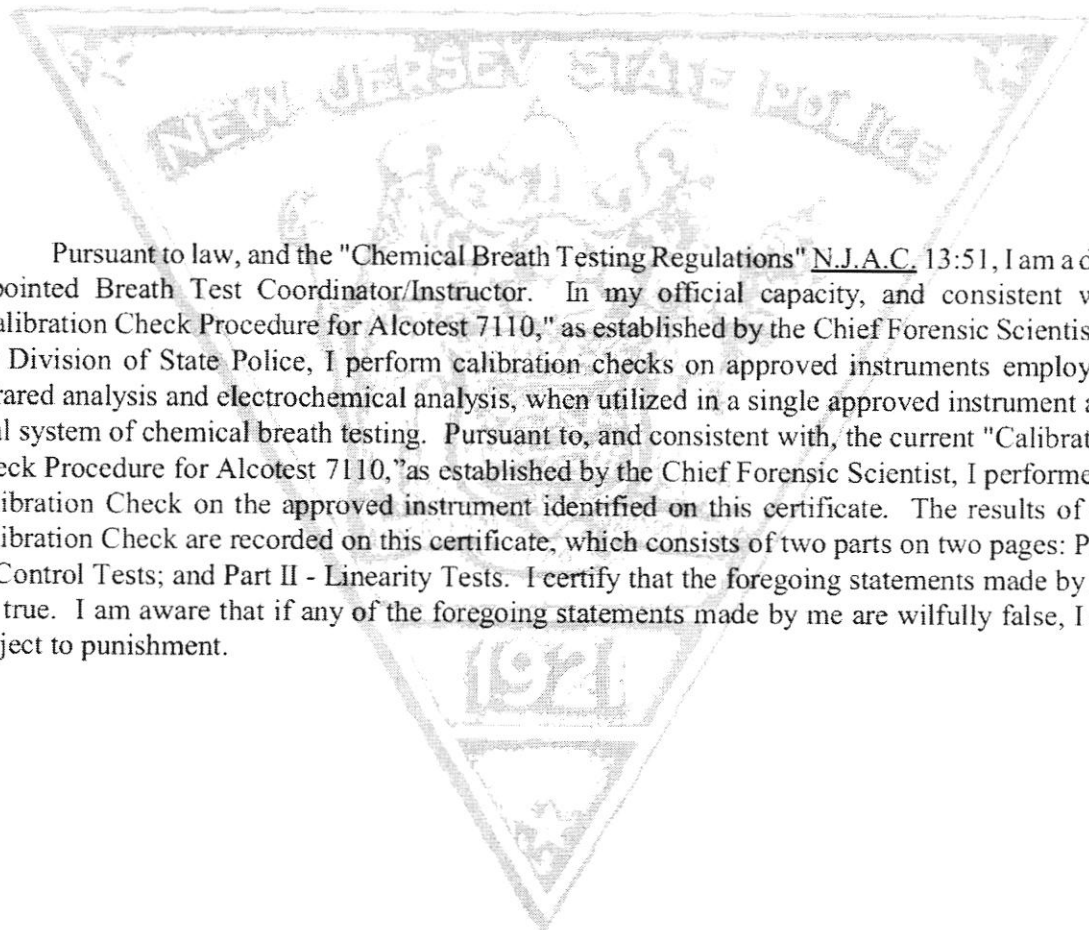

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: PENNSAUKEN TWSP. P.D. Serial No.: ARUM-0051
Calibration File No.: 02684 Calib. Date: 11/27/2017 Calib. No.: 00034
Certification File No.: 02685 Cert. Date: 11/27/2017 Cert. No.: 00030
Linearity File No.: 02638 Lin. Date: 07/11/2017 Lin. No.: 00028
Solution File No.: 02683 Soln. Date: 11/17/2017 Soln. No.: 00281
Sequential File No.: 02685 File Date: 11/27/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 10/10/2018
Solution Control Lot: 16270 Bottle No.: 1055

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:34S		
Control 1 EC	0.099%	11:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:36S		
Control 2 EC	0.098%	11:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:37S		
Control 3 EC	0.099%	11:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38S		


All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: 

Badge No.: 7078

Date: 11/27/2017

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02684 Calib. Date: 11/27/2017 Calib. No.: 00034
Certification File No.: 02685 Cert. Date: 11/27/2017 Cert. No.: 00030
Linearity File No.: 02686 Lin. Date: 11/27/2017 Lin. No.: 00029
Solution File No.: 02683 Soln. Date: 11/17/2017 Soln. No.: 00281
Sequential File No.: 02686 File Date: 11/27/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCB-0001
Control Solution %: 0.040% Expires: 09/19/2018
Solution Control Lot: 16230 Bottle No.: 1237

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCB-0002
Control Solution %: 0.080% Expires: 09/27/2018
Solution Control Lot: 16250 Bottle No.: 0008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBN-0007
Control Solution %: 0.160% Expires: 10/03/2018
Solution Control Lot: 16260 Bottle No.: 0275

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:55S		
Control 1 EC	0.042%	11:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	11:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		
Control 2 EC	0.041%	11:58S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.041%	11:58S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S		
Control 3 EC	0.081%	12:00S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	12:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01S		
Control 4 EC	0.079%	12:02S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	12:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		
Control 5 EC	0.160%	12:04S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.156%	12:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06S		
Control 6 EC	0.158%	12:06S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.156%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:08S		


All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Tpr. II 

Badge No.: 7078

Date: 11/27/2017

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02684	Calib. Date: 11/27/2017
Certification File No.:	02685	Calib. No.: 00034
Linearity File No.:	02686	Cert. Date: 11/27/2017
Solution File No.:	02687	Cert. No.: 00030
Sequential File No.:	02687	Lin. Date: 11/27/2017
		Lin. No.: 00029
		Soln. Date: 11/27/2017
		Soln. No.: 00282
		File Date: 11/27/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	17110	Expires: 03/20/2019
		Bottle No.: 0959

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:56S		
Control 1 EC	0.101%	13:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:57S		
Control 2 EC	0.100%	13:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58S		
Control 3 EC	0.099%	13:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUJ2-143 MRW

Changed By:

Last Name: WATSON	First Name: MATTHEW	MI: R
Signature: <u><i>Tpc II [Signature]</i></u>	#7078	Badge No.: 7078
		Date: 11/27/2017

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:
DDCB-0001

Certification Date: 9-27-17 Technician: BC Re-Certification Due Date: 9-27-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:
DDCB-0002

Certification Date: 9-26-17 Technician: BC Re-Certification Due Date: 9-26-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:
DDBN-0007

Certification Date: 9-26-17 Technician: BC Re-Certification Due Date: 9-26-18

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe: DDXK P2-390 Certification Date: 9-22-17 Next Certification Due: 9-22-18

Probe Value: 104 Draeger, Inc. BC



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8609162

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170428362 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/17 Due Date: 6/08/19
Test Conditions: 23.5°C 50.0 %RH 1014 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	0.000	Y	-0.048	0.052	0.010	>4:1
°C		N.A.		25.003	25.001	Y	24.953	25.053	0.010	>4:1
°C		N.A.		50.002	50.001	Y	49.952	50.052	0.010	>4:1
°C		N.A.		100.001	99.999	Y	99.951	100.051	0.010	>4:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/19/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 10, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of October, 2016.

[Handwritten signature of John R. Leaver]
Notary
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/27/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0492 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 19, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of September, 2016.

[Signature]
Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/04/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0965 to 0.0975 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 27, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali-M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1928 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 17 day of October, 2016.

Notary [Signature]
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer.
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 03/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17110

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1231 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 20, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of March, 2017.

[Handwritten signature of Mary E. McLaughlin]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Matthew R. Watson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 140 OF THE LAWS OF 1966 IN THE OPERATION OF THE A METHOD TO DETERMINE INTOXICATION. ALCOTEST 7110 MKIII-C
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 19th DAY OF August

TWO THOUSAND AND 19th

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>11-8-12</u>	<u>CCPA</u>	<u>Wm Leon</u>
2. <u>7/14/15</u>	<u>CCPA</u>	<u>Adam Gander</u>
3. <u>3/23/17</u>	<u>Lakehurst</u>	<u>Michelle Smedley</u>
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2938 (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Matthew R. Watson
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 140 OF THE LAWS OF 1966 IN THE OPERATION OF THE A METHOD TO DETERMINE INTOXICATION. ALCOTEST 7110 MKIII-C
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Sixteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2938 (Rev. 08/13)

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

3-17-15

SERIAL NUMBER:

ARUM-0051

Draeger Safety Diagnostics, Inc.

PC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDUN53-0338

Certification Date:

10-9-17

Technician:

BC

Re-Certification Due Date:

10-9-18

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUSP2-143

Certification Date:

10-9-17

Next Certification Due:

10-9-18

Probe Value:

103

Dräger, Inc.

BC